




# X-RAY SECTION





## APPARATUS ACCESSORIES—SUPPLIES

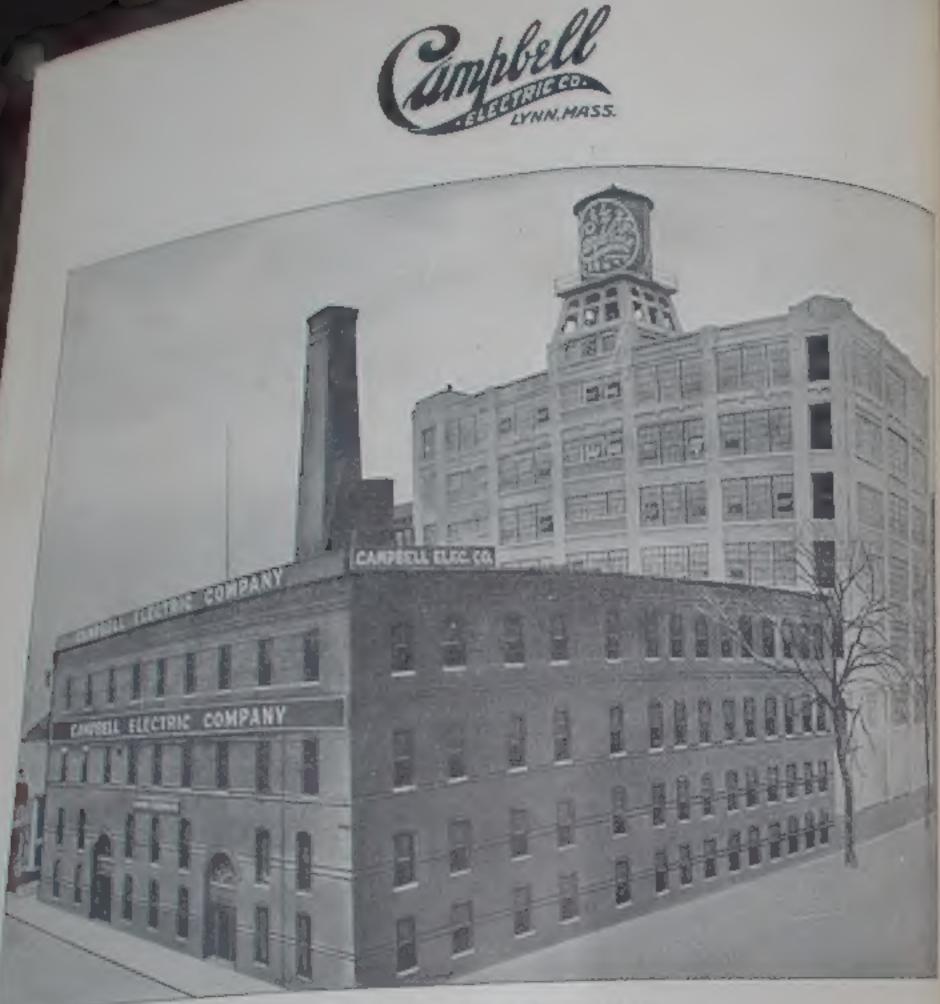

"The Plant That Serves You"

A large and modern factory, designed and constructed with especial reference to efficiency in the manufacture of X-ray and other electrical apparatus.

Our host of professional friends is our reward for past efforts and we shall endower in the future, as we have in the past, to furnish our customers with the best possible apparatus, and what is of equal importance, the best possible SERVICE.







#### INDEX

		PAGE.			P.	AGE
			Coolidge Tubes -			16
Clinix X-Ray Plant		4	Cassettes			17
Crimeal X-Ray Unit -		J	Intensifying Screens .			1.00
Clinette X-Ray Unit		ξ.	Miscellaneous -			17
Clisene Mobile Unit		6	Developing Tunks -			18
Portes Mobile Unit	*	-	Developing Trays			18
OHR-Six Radiographic Unit		67	X-Ray Films			18
BIOLEY LINGSON		8	Dental X-Ray Films			19
Vertical Fluoroscope		8	Safelight Lamps			19
Surex Power Plant		9-10	Developing Powders			19
Deep Therapy Tube Container.	**	11				19
"OH" X-Ray Power Plant		13	Fixing Powders			3.0
Dental X-Ray Unit		14	Film Hangers			
Plate Changer and Tables .		1.5	Dental Film Hangers	-	-1	19
		15	Dark Room Supplies		1.	20
Moters—Switches		15	Exposure Holders	4	-	26
		16	Fluoroscopic Screens			20
Lend Protective Supplies -			Filing Envelopes			20
Time Switches			Physical-Therapy Sect			21
Rotary Converters -	4	10	Layares chessis			




TROLLEY-LESS

COMPLETE



X-RAY UNIT

PLANT

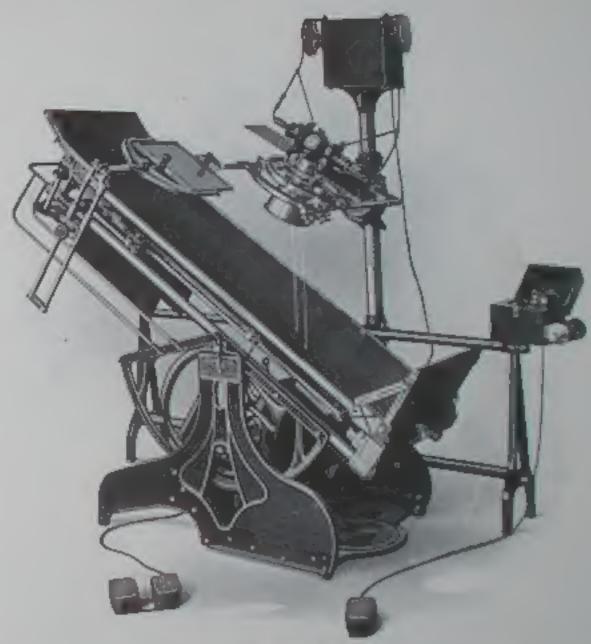

A Most Complete

Radiographic and Fluoroscopic X-Ray Plant Unit

Ample Capacity for Every Requirement

Farnished with or zentant Rucky Displanted Fully Patented

For Prices see Page 1, X-Ray Section







## Clinix X-Ray Plant

Self-excited

COMPLETE

Self-contained



As Illustrated, Catalogue No. 12120

Trofleyless X-Ray Plant



Complete X-Ray Unit

Catalogue

SPECIFICATIONS

2°nice

#### Clinix X-Ray Plant, 110 Volts, 60 Cycles, A. C.

12100 CAMPRELL CLINIX TUBE TIET TABLE ONLY, for use with separate exciting equipment and including Fluorescopic Screen and Halder, Card Reels, Lead Glass Shield or Bowl under Table. First Rest, etc. \$1,0000 12101 Tune Stand Rails with End Castings 12102 Muron Drave (reversible), with Foot Switches ...... 12103 Factoroscopic Transformer, attached under Pable, Reels, etc. 30000 12104 RAMOGRAPHIC TRANSPORMER with Alternings, Reds, etc. 35000 12105 UNIVERSAL NO. SIX TUBE STAND of the Lead Glass Shighlow Bowl, Carriers for Rail Mounting, Platform for Transformer, etc. 310.00

(Continued in next page)





DRIVE CERTIFICATION OF THE COMPLETE OF BOARD SHAPE COMPANIES AND TAKEN	
THESE CERTICAL NUMBER OF THE PARTY COMPLETE SE Indeed above and including adjustable BECKN DIAPRIESCH, etc., for Undergreat as well as all adjustable BECKN DIAPRIESCH, etc., for Undergreat as well as all process of the World - Process of	
	145/8
	3500
	15.0
IN ROLLING CONTENTS for D. C. Operation of Clinic	





## Clinical X-Ray Unit, 110 Volts, 60 Cycles, A. C.



3" to 5" Spark Gap 6-30 M. A.

SHENT

The Ideal Office Equipment





Catalo	EDD HPECIFICATIONS
	The appropriate only
	Cambrier with Control Panel, Cords, etc.
12132	Tital Stanii, counterweighted type
	Luan Grass Smills for Title
12112	Countries X-Ray Tune milities type
12107	First Swerce
12135	CLINICAL X-RAY UNIT COMPLETE as fisted above (Code Word
	"Clinical")
	AUTOMATIC TIME Swinch, Inni type, 0-12, Second Scale
12110	CIPILTIT BELARIE, oil type
12136	CLINICAL X-RAY UNIT COMPLETE and with Band Timer and Cir-
122.00	cuit Breaker (Code Word "Cimi'ac")
1500	
13200	PLAIN TABLE for me with above
12113	FLAT THE TABLE WITH Blocks
12114	FLAT THE BUCKY DIAPHRAGU
12118	ROTARY CONTESTED for Direct Correst



## Clinette Portable X-Ray Unit, 110 Volts, A. C.





SPECIFICATIONS	
Little Fearmers Con., portable type, with Carrying Handle, Cover, Posts,	1,574
Cards: Reels, etc.	£324.
1210s. Courset Cast, with Auto-Transformers, Meters, Rheostat, etc.	
12141 Beautiff Tone Stand, adjustable, with Base, Extension, etc	122/0
12142 CARRYING CASE	0510
12107 Fort Switch	1000
12125 Lean Glass Shire for Tube	1510
12112 Continue N-Ray Terr, cadintor type	Zi(j)
12145 CLINETTE PORTABLE X-RAY UNIT COMPLETE as above (Code	12514
Word "Clinette")	750.06
12119 AUTOMATIC TIME SWITCH, hand type, 0-12 Second Range	4810
12143 Coxx Hotzer with two Cones	250
1413 Casseer, Hv14 Buck	17.31
14514 INTENSITYING SCHEENS, 11x14 pr	28.14
14411 Cassery, Sx10 Buck	
14512 INTENSERVING SCHEEKS, Sx10 pr	135
15170 HAND FLUOROSCOPE, 5x7	1410
	25.14
13502 RULEY DIAFRIKAUM, flat top, 12x12 (for 11x14 Films)	175 00
the partition type	100.00
POWERFUL PORTABLE PRAC	TICAL



### Clinette Mobile Portable X-Ray Unit

A combination Portable X-Ray Unit and Mobile Office or Ward X-Ray Unit. Can be easily transported to bedside of patient and serve as an efficient compact Mobile Unit in the office or ward.

Catalo	gue SPECIFICATIONS	Price
12140	Total Posts	
	Cords, Reels, etc.	
12106	Control Case, with Auto-Transformers, Meters, Rheostat, etc.	115.00
12132	Tem Stano, Counterweighted Type	150.00
12144	Monne Base, with Cable, etc.	83.00
12107	Foot Switch	15.00
12125	LEAD GLASS SHIELD for Tube	
	Coolings X-Ray Ture, Radiator Type	
	CLINETTE MOBILE X-RAY UNIT, as listed, complete (Caste word	
	Mobette)	
12141	BRACKET TURE STAND, Adjustable Type, with Base, Extension, etc.	
12142	CARRYING CASE	40.00
12147	CLINETTE MORILE X-RAY UNIT. as listed, Complete with Bracket	
	Tube Stand, and Carrying Case for combination home and office use \$	985.00
12148	Same as Amove, but with Automatic Hand Timer (12119) and Circula	
		00.800





## Portex Mobile Hospital X-Ray Unit



PORTEX

SPECIFICATIONS Catalogue 12150 PORTEX MOBILE HOSPITAL X-RAY UNIT COMPLETE as listed (Code Word "Portex") ...... 890050 12151 PORTEX MOBILE HOSPITAL X-RAY UNIT COMPLETE as listed (Code Word "Portal") ...... 8990.4 



OHR-Six Radiographic Unit



#### TYPE OHR-SIX

(Overhead Transformer on Rails with Number Six Universal Tube Stand)

Catalo	gue SPECIFICATIONS	Price
12104	TRANSFORMER, with Mountings, Reels, etc.	\$350.(x)
12105	UNIVERSAL No. SIX TUBE STAND with Lead Glass Shield or Bowl, Carriers for Rail Mountings, Platform, etc.	
12106	CONTROL CASE, with Auto-Transformer, Cords, Rheostat, etc.	113:00
12101	TUBE STAND RAILS, with End Castings	\$0.00
12112	Cool loge N-Ray Tune, radiator type	125.00
12107	Fort Switch	15(8)
12155	COMPLETE OHR-SIX X-RAY UNIT as above (Code Word "Oversax")	965,00
12109	AUTOMATIC TIME SWITCH, hand type, with Stereoscopic Reset Stop	-83.00
12110	CIRCUIT BREAKER, oil type	45.00
12156	COMPLETE OHR-SIX X-RAY UNIT as above and with Time Switch and Circuit Breaker	1,060,00





## Florex (Fluoroscopic) X-Ray Unit

	SPECIFICATIONS	15
Catal	одие	Price
12130	TRANSFORMER, with Posts Steener, Meters, Cords, Rheostat, etc.	270,00
12105	CONTROL CASE, with Auto-Transformer, Meters, Cords, Rheostat, etc.	115.00
	AND ADDRESS OF THE PARTY OF THE	15.00
12159	MORILE HASE for Control Case of Attachment Bracket	50'00
12160	MORREE HASE for Control Cast FLOREX (Finoroscopie) X-RAY UNIT COMPLETE as listed (Code Word "Florex")	395,00

## FLOREX X-RAY UNIT

## Vertical Fluoroscope

Catal	logue SPECIFICATIONS	Price
13150	The Congression of the Control of the Change of Class of the Class of the Control	
12112	Coolings X-Ray Ture, vadiator type	125.(1)
12160	FLOREX (Fluoroscopic) POWER UNIT	395,00
13151	"Flovert")	950.90
14010	LEAD RUBBER PROTECTION GLOVES, J	10.06
14012	LEAD RUBBEE PROTECTION APRON	12,00
12121	ROTARY CONVERTER for use on D. C	100 00

Note: For Tilling Fluoroscope prices, see Clinix List, Page One, Catalogue Number 12100.





For operation on 220 V., 60 C., A. C.



200,000 Peak Volts
0-200 Milamps.



DEEP THERAPY

POWER PLANT



For price list, see next page



## Surex Deep Therapy Power Plant

SPECIFICATIONS	
Catalogue  (2501 High Texsion Transformer, oil insulated type, including Insulators	( rice
and Motor Base. 220 Vi. Del Vi. Del Vi.	300:
12502 Syxensonous Motor, double disc type, with Collector Arms, Shields,	2400
elc.	285 (4)
12503 Control Tamer, with Auto-Transformer, Meters, Cables, Polarity In- dicator, Circuit Breaker, Resistor, etc., mounted on ball bearing casters	
with connections	100/6
12504 FILAMENT TRANSFORMER, with connections	1955
12184 AMMETER for Filament Circuit	45 <sub>Ju</sub>
12181 MILLIAMPEREMETER, Double Scale 0-20:0-200	
	65.16
12507 SUREX DEEP THERAPY POWER PLANT COMPLETE as listed	
(Code Word "Surex"	2,295,56
12520 TREATMENT TIMER	35.1%
14230 SINGLE DECK BRACKET for Overhead System (tubular type)	103,
14231 38 inch Brass Turing, per foot	4
12157 Cord Reel, Andre	12.m
12158 CORD REEL CATHODE	16.96
12161 CATRODE CONNECTOR	3.5)
12165 High Tension Spiege Gap, 225 k. v. a	265.m
12512 Coolings Tube, Deep Therapy Type	260 m



### Deep Therapy Tube Container

Catalo	gue SPECIFICATIONS	Price
12508	DEEP THERAPY TORE CYLINDER, rotating, with H. T. Iremistors \$1	(VA) (E)
12509	Tone Cylister Carriage, with Tracks and Performently Adjustable	
12510	DEEP THERAPY TUBE CONTAINER COMPLETE as above (Code Word "Zeplin")	
12511	SAME AS ABOVE, but with Main Carriage Manually Adjustable to raise and lower by means of hand-operated lever (Code Word "Adlin")	
12512	COOLIEGE N-RAY TUBE, Deep T empy Type	361.00
12514	ADJUSTABLE TYPE TABLE, recommended for use with Cat. No. 12516 Tube Container	225.00
12515	PLAIN TABLE, with Cushions	. 15000
12516	PLAIN TABLE, with Cushions, and with three hinged sections	
12517	BLOWER MOTOR for cooling X-Ray Tube in Container	30.00
14010	LEAD RUBBER PROTECTION GLOVES, pr	1000
14012	LEAD RUBBER PROTECTION APRON	12.00
12137	SHEET LEAD, per 1b	35

Note: Price on Deep Therapy Tube Container is for Plain Flows (Grey, Black, Dark Red). For Mahayany or other Special Flows, and \$85,00 to List Price.







Leading Roentgenologists and Institutions throughout the world use and second Campbell Roentgen Equipment


Pictured here are two of the thousands of institutions equipped with our apparent







Model "OH" X-Ray Power Plant

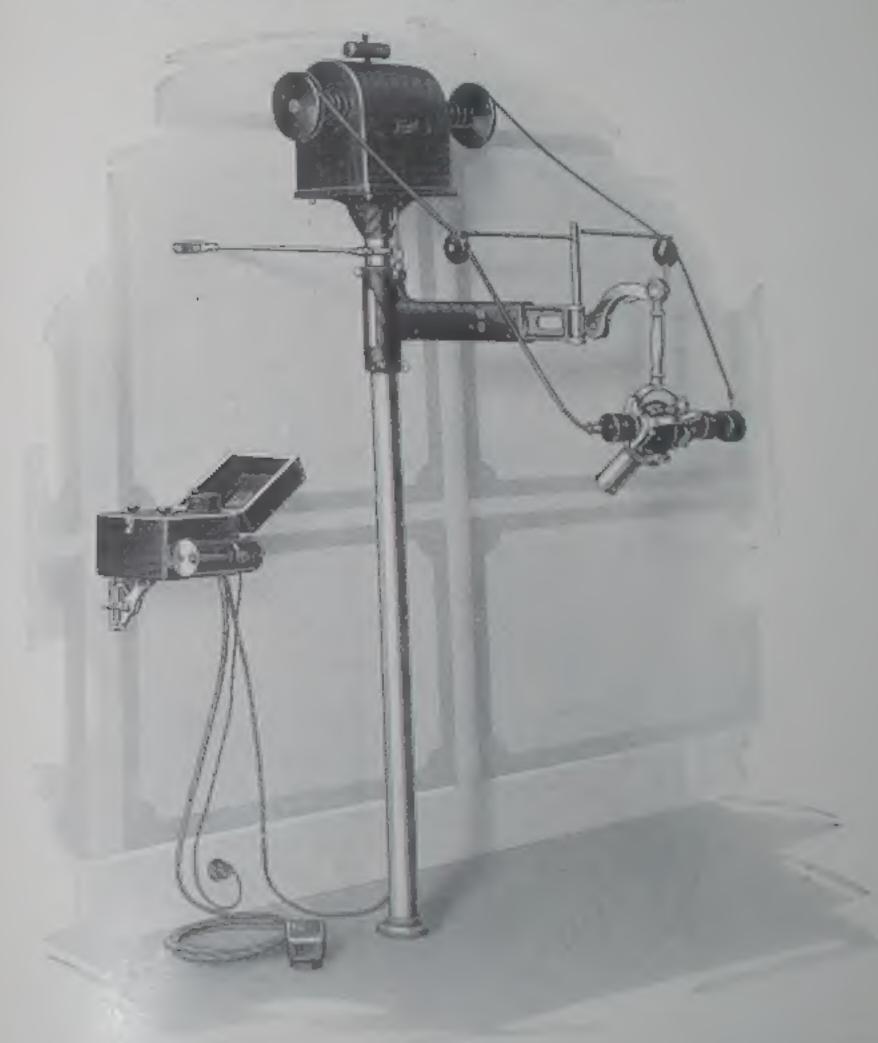

Catalo	gue SPECIFICATIONS	25551
12245	TRANSFORMER with Mountings, etc.  CONTROL CASE, with Auto-Transformer, Conds, Rheostal, etc.	
12107	For Switch	175
12171	TUBE STAND, Crane type for wall mounting LEAD GLASS SHIFLD for Tube	7 7
12112	COOLINGE X-RAY TUBE, radiator type MODEL "OH" X-RAY POWER PLANT COMPLETE as listed (Code	
12170	Word "Crano")	893.

13



# Campbell Dental X-Ray Unit

Catalogue

1977 - Level and Catalogue Region Costers, Americana Proceedings

1977 - Catalogue with Morein High Tension Post, Casters, Americana Procedure

1977 - Catalogue Communication of Table and administration of Communication Communica

For use on 110 v. 60 c. A. C. 65,000 Velts, 0-10 M. A.



Priced Right

\$625.00 Complete

Built Right

Campbell



## Meters - Switches

[2]85 Value of for [2]84 Value of for [2]85 Value of for [2] [2] [2] [2] [2] [2] [2] [2] [2] [2]	Filament Coccurs  100 K. A Commence  120 C. Schnetch	Present States States States
Man Hann Tray or	MASO CHARLES TO STATE OF THE STATE OF T	15 o Tison 65 on
	Tables	1278
	4*3557444	

Catalon	SPECIFICATIONS	
	THE VEY RADBURGAPH DE ANDER DEALERS PART.	Price
12514	ADJUSTABLE TVIT TABLE for use with Deep Therapy Drum No. 12510	33
. 1515	PLAIN TABLE with Cushions for use with Deep Therapy Dieno PLAIN TABLE with Cushions and with three hinged sections.	14519

#### Bucky Diaphragms

FLAT TOP	CL RV	100
17x17 11x14	CLES TO TO	17

Catalo		12
12176	CURVED TOP BUCKS DIAPHRAGM for LINES and Section of the party	Price
12114	Fig. Tor Bucky Dimpirkagn for 17x17 and a second Electric Contact Device and Compression 10x03	\$250.00
13502	Fixe Top Birchey Diaphrams on 11x14 and 5 11x14 and 5 12x14 Bakelite Top, Compression Band, Corney Social	
13503	Corner Post Rope for Hyld Bucky	
13504	CASTING AND POST (or Head Charm	46.1
13501	Electric Contact Device for Color Colors	**



12111 Francescopic Blocks Dynamics of




Lead Protective Supplies	
Untalorge	
12128 Constant Series for British Luber Commission Series for British Lube	$\mu_{\rm rice}$
12487 July 15 Ass. Only Bowl	35214
	Burn
	2.36
	11111
12437 for an above the furth risade, per The succession and annual and an accompany	12,66
	80
Time Switches	
Catalogue SPECIFICATIONS	
12109 Action vite Time Switten, two contact style, and with Stereo-Reset, 0-12 sec	Price
12119 SAMP AS 12109, without Stereo-Reset Device	\$5316
12120 Same as 12110 except has three contacts so as to open and close main	486.
circuit through protective resistance. Maximum rating 10 M. A	48,06
Rotary Converters	
Catalogue SPECIFICATIONS	0
12118 ROLLEY CONVENIER, 140 v., D. C., 110 v., A. C., for 30 M. A. units	Price \$265.0
12128 Savir vs 12118, 220 v. D. C. to 110 v. A. C	350.0n
12:21 Region Cenamerra, 110 v. D. C. to 110 v. A. C., for 10 M. A. units,	
Coolidge Tubes	
Catalogue SPECIFICATIONS	Price
1202 Coolines Tees Radiator type, 30 V. A	\$125.00
12138 Centrace T. and Radiator type, 10 M. A. J.	125,00
12178 Continus, Tens. Dental type, Right Anche	125.60
12168 Coolings Tree, Curveral type	125.00
12512 Commission (1946-200-3) A. type	250.00
1973 Control Steel Deep Theology type	260 (0)



#### Cassettes

SPECIFICATIONS	
Catalogue  14410 CASSETTE: 5x 7 size	Price \$10.00
14411 CASSETTE: SX10 Size	13.50
1.1412 CASSETTE, TON 12 SIZE	15.50
1.1.13 CASSETTE, TIX 14 SIVE	17.5
1944 CASSITER, 14x17 Size	10.50
14415 CASSLITE. 17x17 size	2100
14416 CASSETTE, 14x17 size, pneumatic	25 (6)
Intensifying Screens	
Catalogue SPECIFICATIONS	Price
145081 587 smglc	3 2 3
14501 613×8×5 single	5 4
14502 8x10 single	8 1
15303 405.12 single	12 0
12504 11x14 singl	1
14505 44x 17 single	24.00
44510 5×7 double, per pair	: *
[4541 6] (x81) double, per pair	8.3
[14512] Sv10 double, per pair	\$
14513 10x12 double, per pair	22. 4
14514 Hxl3 double, per pair	7
44515 14x17 double, per pair	-13
Missallamanus	
Miscellaneous	Price
Catalogue SPECIFICATIONS 14015 Eastman N. Ray Viewing Box for 14x17 Films	\$12.89
14016 HASTMAN N RAY VIEWING BOX 101 8x10 Films	0.00
14017 Laxo Liberto Box for 14x17 Film	10.00
13018 There Diegra Firm Cites	191
14019 EASTMAN DENIAL FILM SAFE	300
12517 Browns Moros for Deep Cheraps Cooling System	20.00





#### Developing Tanks

SPECIFICATIONS

gui	* Charles
Particular description of the second of the	somparing .
The 17 Chaire and the summer and the contract of the contract	Street, and the Bart
A complete with compact facts, complete with connect	tions
Taxas Day Commencer Day as the State of the	
20 10 11 12 12 X 2 X 2 X 2 X 2 X 2 X 2 X 2 X	The second secon
Samuel Control (1986) - State Self and the control of	Service Control of the Control of
Secretary I System FASKS, 47 28 [43, 820] minimum	Control of the Contro
1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1	The state of the s
C. Dostones Task other	
Total CLY AND THE DESCRIPTION OF SERVICE	Compartment
C10 Piless, with July	10r
can as 15108, except without lids in amount	
	The state of the s
	pour rate 1.8 years Developes. Task othered profession 1.8 years fax is complete with connect profession 1.8 years fax is complete with connect profession 1.8 years fax is 21.88 years fax years fax is 21.88 years fax years fax is 21.814 years fax is 1.8 years fax years fax is 1.8 years fax is 1.8 years fax years fax is 1.8 years fax is 1.8 years fax years f

Catalo	igite	SPI	ECIFICATIO:	NS	
1 - 1 2	District Const	Francis Trays	$\zeta=5 {\rm k} Z$ , each	***************************************	$P_{\theta_{R_{i}}}$
15111	Programas	Examelia Leave	$z=7\pi 9$ , each	***************************************	81 3:
1-112	Programas	FX CAPTED TRAYS	, 8x40, each		1:
15113	Popular vis	Example Travs	, 10x12, each	***************************************	17:
1 1 1 4					2:
15115	Pokertain	EXAMPLED TRAVS.	14x17, each	41974	3.
				A CONTRACTOR OF THE PROPERTY OF THE PARTY OF	

## Eastman Duplitized X-Ray Films

Catalogue			SPECIFICATIONS	
(51)6	357	per dozen.		Price
15137	$f(x,y(S)^{-1})$	per dozen.		\$ 120
A 47 4 1 5 1 1	21.5	10. 100 100 100 100 100 100 100 100 100	Notice to the College of the College	
13170	100.12	Seg. Cozen.		3.
151 (6)	11814	per dozen.		3.5
13121	13/17	san di sen-		fire.
				100

#### Eastman Safety Duplitized Films

Catalogue		SPECIFICATIONS	Pr.c.
17111	5.7	ger dozen	\$ 100
17,23	Q 35 5	- Let Pozen	3,
			1.
11141		the developing the second seco	421
15126	11 17	pro dozen	70
15127	14%17	per dozen	121

Some In malering specific "Super Speed" or "Contrast,"





## Eastman Dental X-Ray Films

Catal	ogue SPECIFICATIONS	
15130	. Removitaro "A", per padana	Price
1513b		\$1.18
[5132	Example Fast (Non-Curling) "Bitt, per package Righting "C", per package	1.30
15133		1.40
15134		7:
15135	1111 11 11 11 11 11 11 11 11 11 11 11 1	7.1
15136	Burs Wing. Type 3, per pachage	: 25
**		1.75
	Safelight Lamps	
15137	BROWNIE SAFELIGHT LAMP	
15138	13/15/19/19/19/19/19/19/19/19/19/19/19/19/19/	8-175
15139	The state of the s	1.4
45140	the property of the print of th	
15141	Wrater, No. 2, without Slide	1000
		8000
	X-Ray Developing Powders	
	a a coping I owders	
15142	solution 12 02. ready to the	
15143	No. a package sunctent to prepare one redlor sends and a	\$ 14
15144	No. 4 package sufficient to prepare five gallons ready to use solutions.	
	X-Ray Fixing Powders	
15145	No. 3—To make one gallon solution	
15146	No. 4-To make five gallons solution	3 .
		2.5
	X-Ray Film Hangers	
15147		
	5×7	\$ 73
15148	6!(x8);	83
15149	8 <sub>8</sub> 10	1.25
15150	-10x12	1.5
15151	11x14	1.73
15132	14x17	2.8
	Dental Film Hangers	
7.74.		
1210.	10 Clips	,
12363	40 Clips, Short Model	2.50
12164	14 Clips	1.50



### Dark Room Supplies

SPECIFICATIONS

Palatogue	
Table Discon President and address four Haugers and and a second of the	le <sub>p</sub>
1318. The Control of	L
1315. The visit of the property of the state of the size, with Lid with a size of the size	٠,
	2:
	7:
[4] And the companies of the companies o	:
*1 * 1 * 1 * 1 * 1 * 1 * 1 * 1 * 1 * 1	
The state of the s	0
The state of the s	
the Physics Press Vinexes for use with Bit Wing Technique, per 100	

#### Exposure Holders

#### SPECIFICATIONS

((8) 8)	alfatra.			
1 17 -	4 . T	street much	 	ria
13,575	1 18	2100, Carrie		
316.5	85,10	-r. c. cm n	 	
1 - 166	- 10x 1.7	Saute (Cart)		
(8167)	$-11\sqrt{D_{z}}$	Six, card		
15004	13847	$s_{t+1} = c(p^{\alpha})$	 	

#### Fluoroscopic Screens

Catalo	SPECIFICATIONS	
15370	55.7 Havin Fair oaoscore, mounted and a man a man	$P_{\theta \eta_{t}}$
13171	The process of the standard from the control from the standard fro	
151713	[4] Criminal OPE [50 BOLD CONTO) [282] [40 a.	
15173	Fr. mansk opp. South S. CONTS, SNOT	,
15177	(i) paper oper Sowiek ONIN, 19812	
15175	Jorganian Segret Over, Hylkanan and an annual and annual	1. 1
15176	Tripoloscom Search Onta, 42546	25 -
15177	Introductions Scatter Only, 14v47	fer 1

#### Filing Envelope

Catali	wite	SPECIFICATIONS	1'0
1317	3.7	(per 199)	5
15179	$(i_1, \dots, k_n)$	. per 100	
$(\gamma_{ij})_{i \in I_{ij}}$	20.76	, per 100	
(315)	That	per 100	
jejy <u>o</u> r	17913,	per 150	
15383	14, 17,	per 100	



# PHYSICAL-THERAPY SECTION



# APPARATUS ACCESSORIES-SUPPLIES







#### INDEX


	PAGE
Compared An Diathornix Compa	23-25
Wide but Disberny (Portab	le i 26
Martin of the Englishman	27
Acceptine for Paint army a Norrable	op. 28 -
Romany Conventions	28
Time Switches	28
MilManueller - Commission of the Commission of t	28
Auto Condensation Chair	294
Anno Condensation Pad	28
Pour Switches .	28
Variety Death rank Charges	
Compliance Electrode	

Entreration Electrode	PAG
Distillering Metal	2
Vacuum Electrodes	į
Dirahermy Electrodes	:
Alpine and Kromayer Lamps	1
Literior Lamps .	S.
Reserve Burners	2
orders Lamps	٠.
Applicators and Spare Paris	34
Corse Wave Generator	Ą.
	33
Vir and Vacuum Apparatus	31
Vir and Vacuum Accessories	



## CAMPBELL DIATHERMY

MODEL "CA"

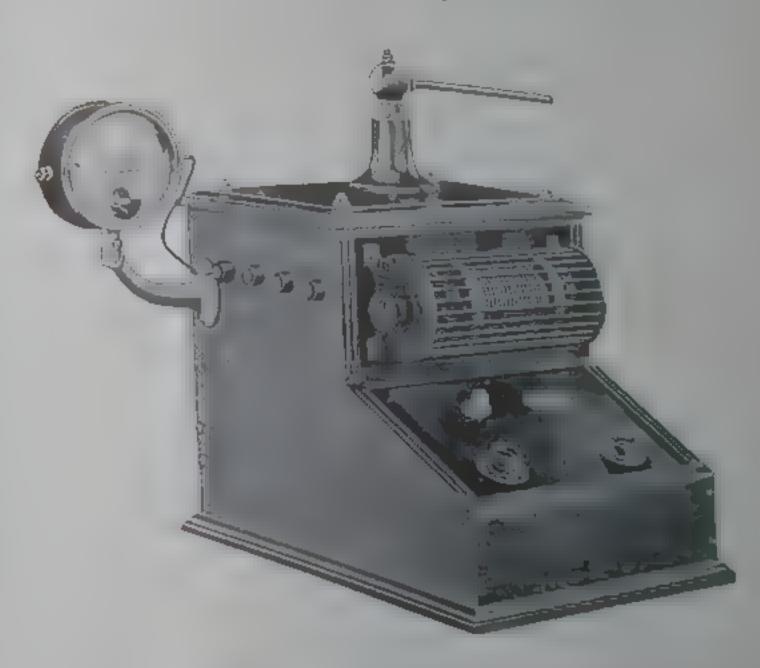


#### SPECIFICATIONS

Adjustable Frequency (Stimulating or Sedative) Dual Control Selective V ... Variable Penetration — Fully Adjustable Compensating Spark Cap (Quie No. 1) Flexible Regulation.

Most Powerful Diathermy Rull!







Campbell

MODEL "CA" DIATHERMY




ILLUSTRATED WITH MOBILE TABLE



MODEL
"CA"
DIATHERMY

Beautiful Design

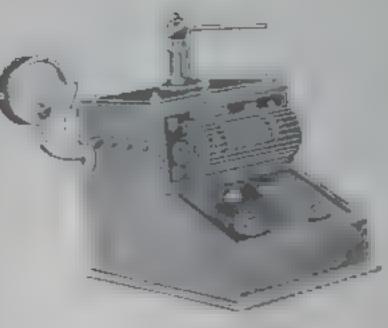

MODEL
"CA"
DIATHERMY

Esticient Design

## Model acva-

	Price
SPECIFICATIONS on c. A. C., with Cords.	
Catalogue  Catalogue  16101 MODEL "CA" DIATHERMY for use on 110 v., 60 c., A. C., with Cords.  Oudin Terminal, Meter Bracket, Handles, etc. Brown mahagany, black	5350.00
Oudin Terminas, and trinsmings	e de la composition della comp
16102 MILLIAMETER, Double Scale Courself as listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT as listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT as listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT as listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT as listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT as listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT as listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT as listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT as listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT as listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT as listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT as listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT as listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT as listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT AS listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT AS listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT AS listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT AS listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT AS listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT AS listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT AS listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT AS listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT AS listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT AS listed, ready to operate (Code 16108 MODEL "CA" DIATHERMY OUTFIT AS listed, ready (Code 16108 MODEL "CA" DIATHERMY OUTFIT AS listed, ready (Code 16108 MODEL "CA" DIATHERM (CODE 16108	393,00
16102 MILLIAMETER OUTFIT as listed, reads 16108 MODEL "CA" DIATHERMY OUTFIT as listed, reads Word "CameC")	-: -:
TORRESTOR OF USC WHILE STORY	
16103 MODEL "CA" DIATHERMY CLAMPS, set and a listed under Cat, No. 16100 16105 MODEL "CA" DIATHERMY OUTFIT as listed under Cat, No. 16100	112:00
16105 MODEL "CA" DIATHERMY OUTFIL as more "Camea") or or or and with Cat. Nos. 16103-01 (Code Word "Camea")	0.50
16106 Feligerator, set complete	1.
16107 Coagulation, set complete an	-
CONTRODIC HANDIA OF THE PROPERTY OF THE PROPER	
TOTAL MARCHEM ELECTRODISC SET OF SIX OF THE TOTAL	100
GOLD COLUMN BURGINGS	
16113 Docum Evi Ernetrom	
16113 Documents of the Color of	243°44



#### Model "CE" Portable Diathermy

e atalog	SPECIFICATIONS	Price
	MODEL "CE" PORTABLE DIATHERMY with Cords, Oadin Terminal,	
16120	Milliameter, Spark Gap, etc., ready to operate on 110 va 69 c., A. C	\$265.00
10193	VACCE DIATURRAY CLAMPS, Set	22,00
16106	ferrance considere	6.50
16107	Costa Lyron, set complete	10,50
16408	Print Switch a management and an arrangement and an arrangement and arrangement arrangement and arrangement arrang	17.00
16109	A SOLVEN Perfergons 11 years	4,50
16110	Victor Programmes Set of St	7.30
16124	Areas Coxpression Par with handle	20,00
16121	MODEL PUET PORTABLE DIATHERMY COMPLETE as listed (Code	
	Word "Cepurt")	315.00
1rd03	Months: Fallin nor use with above administration of the box	. 451K
16125	THE RESERVE OF THE PROPERTY COMPLETE AS USED AND	3
	including Mubile Table (Code Word "Cetal")	020.0

# Model "CE" Portable Diathermy

Complete

Compact

Efficient

Easy to Carry

Mest powering Portable Diatherony budy

Note: For currents other than 110 v. 60 c , it. C., with for anothers.



#### MODEL "CI" DIATHERMY

DUAL CONTROL

Admistable Frameway

Selective Voltage

and

Variable Penetration

SPARK GAP

Compensating Type
Steady, Quiet and Fully
Adjustable

EVERY
MODALITY
EFFICIENTLY PRODUCED

ALL MODALITY

Terrogal (breed top)
Automatic rest Weating Regis
(b)
Heavily breedated top).

CABINET

Mahogare Could be trade.
Members on the Color of the Sterile.

MOST POWERFUL DIATHERMY BUILT


1604 VACUE DIATHORAS CENSUS, set-

Special Price for Complete Dutht when indered logical





## Model "CH" Portable Diathermy



Designed for Home Use of Patient

Caful	forgest-	
18111	A. C. complete with Cords, Oudin Terminal, Spark Gap, Diathern	
	Note: All accounts according to the near with above with Figure 1. Combined to the state of the	. 81 (5,0n
	Rotary Converters	
Cataloj	gue SPECIPIO CONTACA	
12121 46138 16138	ROLLY CONGRESS, More D. C. to 110 v. A. C., 10 supperes	Price \$10000 173.00 75.00
	Time Switches	
Catalogi 12450	SPECIFICATIONS  1. TO NO. JUNES. Automotion	Price S.Con
1 - 1 - 1	1 Control Control Marine Clock Type	344
	Miscellaneous	
Catalogy	e SPECIFICATIONS F	Prior



## Vacup Diathermy Clamps

SPECIFICATIONS	Price
SPECIFICATIONS	\$22,00
SPECIFICATIONS  SPECIFICATIONS  PARTY VACUE DIATHERMY CLAMPS, per set	2.191
ONE PARK, Large Discs	5,50
Ove Pars, Large Discs	1.0
oys Pyra, Medium 1960 s.m. and	275
J. O. Osay Short Spreader	1.75
of the Osto, Long Specialist and announced statement of the control of the contro	1.0

#### Coagulator Set



Catalo;	SPECIFICATIONS ELECTRO-COAGULATOR, per set	Price \$10.50
16107	ELECTRO.COAGI'LATOR, per set	- 1
16,708	HANDER, only	1.20
1/Ches	Costs, insulated	- 4
[46,5] [1]	Correct Links. Passes	- 5
19315	Nerota, Point Type	
	Fulgerator Set	

	Insulated Positive Action Type	Proce
atalog	SPECIFICATIONS	 86.70
6106	ELECTRO-FULGERATOR, per set	 =
6213	Private viole Handle only the more than the second	
6214	NUMBER   Knote   Fylor and the man and the	
5일 8 년 6월 6 년	Name   Ball Type	 -

#### Diathermy Metal

16220	DISTREBUT	METAL	per	ral)	<b>**</b> **********************************
-------	-----------	-------	-----	------	--

Roller
Free with full
roll of metal

Q2 ×

1900



Cords \$3.00 per set Cat No 18000



Action to the second of the se

I the company of the company



# Model "CH" Portable Diathermy




Designed for Home Use of Patient

Price



#### Vacuum Electrodes



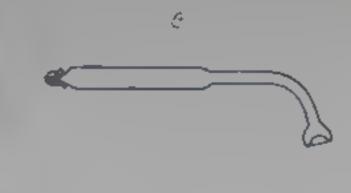

Catalos (6112 (6113	SPECIFICATIONS  SUSCITE FOR THOSE COMMERCE COMME	Price \$ 3.00 100
16110 16110	Vaccinal Errenson Having	0,50 7,50
16221 16222 16223 16223 16225 16225	Service Freedom, Plain Type  Carriery Freedom, Plain Type  Freedom, Plain Type  Freedom, Plain Type  Kreich Freedom, Plain Type  Viscont Freedom, Plain Type  Viscont Freedom, Plain Type	1.50 1.50 1.50 1.50
16231 16233 16333 16233 16234	Toron r. Engergood, Insulated Type	200 200 250 200 200 200
1625 	7 — Сурптиоров — Интегроор — поста принцений поста поста 8 — Сурти System - Интегроор — поста п	1.50
102 102 102 102 102	Properties Errespons, Dental Type	





## Special Diathermy Ele

Catalogue 22250 Merrae 22251 Merrae 22252 Merrae 22253 Connes 22257 Connes	PROSERVICE PROPERTIONS  PROSERVICE PROPERTIONS  VALUE OF THOMS Explained  VALUE OF THE PROPERTION OF THE PROPERTY OF	P
	* * * * * * * * * * * * * * * * * * *	:

## Alpine Sun Lamps Alternating Current Equipment, Lines

	The state of the s	
Cata	logue Sparser, Hn C	
22031	On movable floor stand, complete with a	
22033		Proce
22035	of goggles  On ceiling suspension, complete with transformer play pair of goggles  Complete, with special mobile base LAMP without transformer to complete.	. 1 DC#
*****	pair of goggles with transfer with	
22210	Complete, with special mobile base  LAMP without transformer to complete combiners  2022 to work	
22040	LAMP without transferons base many	* 12 .
22041	LAMP without transference to complete grant a second	
		1
	For other than an inner on one and direct to the	
	Lame without transformer to complete combination as 22022 to make combination unit on one stand for direct and For other than the Cycle equipment, add \$5000.	
	Alning	274

## Alpine Sun Lamp

	Direct Current Eurica Lamps	
Catalo	ague Equipment 11	
22030	On movable theor stand SPECIFICATIONS OF DOLLARS	
12015.2	Attacked a fine of the state of	
2002	On wall bracket, complete with rheostat, place to complete with rheostat, place to pair of goggles.  Ceiling suspension lamp, complete with rheostat, place to pair of goggles.	Pela
2034	Ceiling Commission With Physical Physics	
	goggles complete with rheostat, pluz complete with rheostat, pluz complete with rheostat, pluz complete with rheostat.	115
2036	Movable flows and and the with themself	
	Kround and John Louis, as let	-

2036	Pair of goggles Complete with a line of			
44,074)	Movable theor stand lamp, without theostal lamp without stand to complete combined	1 1111		
2000	Kromayer Lamp (to complete combination 25%)		· · · · ·	
47,763	With without group complete combined and the			
	Lyar without stand or three-star for attactonomy			
	The South Court of the Court of the Court of			

## Kromaver I

Catalogue	Alternating Current Equipment, USA SPECIFICATIONS		
Policinal Company		2.3	
արկերդ	The later than the state of the		Cong
Philosophics (	her protection windows and the		\$
Seling Sendal	Thirty self contained conting action.  Self Contained Unit, Salt contained for the contained of the containe		
	Property of the Contract of th		· ·

For other than of twelv company



## Kromayer Lamps

	Down the SpecificATIONS	Price
hitalest	the state of the first of the state of the s	
	The first of the first of the first part of the first of	385 00
	The contract of the contract of the property of the contract o	715 00
CHINA	The first property of the contained cooling section, with an area of the first property of the contained from the contained fro	
Open	The way to be the property of	385 00
	probable with temporary temporary probability by the probability of th	520,00
1.	model Control Control Control	
	Thermour: Cherene Equipment, 130 V., or 220 V., or Cy SPECIFICATIONS SPECIFICATIONS	l'rice
Catalo	SPECIFICATIONS  SPECIFICATIONS  Sun Lamp, complete, each confound of kremaver Lamp and Alpine Sun Lamp, complete, each confound on kremaver Lamp and Alpine Sun Lamp, complete, each on again to stand and using same transferour. Pachasive of appearance of an again of sun and alpine Sun.	205,00
		930.00
25.713	Professional and two morights and using Eventures Econoxer Burner	
	Rad and China Charge neck without extra clurtee when si space than Camp or	1,120.00
12213	Head and Preport attressment without cause charge when so spectices in place of the Goose need without cause charge and Alpine Sun Lamp of Postsuk Combination Unit Knownver Lamp and S50,00 to price hop other than 60 Cycle equipment, add \$50,00 to price	
	Carbination Lamps	
	The state of the s	Price
	**************************************	ıt.
Catul	logue    Consists of Kromayer Lang. complete a consists of Kromayer Lang. complete a consists of Kromayer Lang. complete a consist of Kromayer Lang. complete.	S 610,00
	The transfer of the control of the c	111
(20	to tentificate and two times are supported supported to the support of the suppor	(61917)
	arplantation from the state of	1 6 33 1 1 20 1
× 1 + 1	to December into the land of There Completes the State of the Consection	KI Marin
277	20 Postable Service with two merigids and using the Krongwer Burt	act
	Provide Selection after two uprights and using Kromayer Burn Sun Lames of their with two uprights and using Kromayer Burn Rack and Phonon admissment will be from shed in the Kromayer Burn on the root the Gorse neck without extra charge when so specified	
	Luxor Lamps	thrice
		hug. 3180.91
C at	specific ATIONS  stategue  the constraint of a pair of a pair of a pair of the state lattice with the state of the pair of the pair of a	ands
	the constraint of property of the state of the party of the state of the plug. It is not state of the party of the state of the state of the party of the state of the state of the party of the state of the party of the state of the party of the state o	213.0
	The state of the s	
		Pri
	En Appending Currents, 181 Cy.	
	CIPMINITE I CANADA CONTRACTOR CON	255
-	'atalogue'  College Complete and Experimental Direct Corrects, 110 Value 220 V.  For Direct Corrects, 110 Value 220 V.	
	the supplied of states and the supplied of the	175



## Sollux Lamp

	Apperate universally on A. C. on L	-aups	-
Catato	PRING OF THE PRINCIPLE	In order	
32217	From Style Lyn Christian	ATTORNAL TALE	
	**Perate universally on A. C. or D. C.  **Rue Style Lyne (Dong W. Bullo, Sylve Color Killa) on for local or Figures for use with floor stand type.  **The Camparase Figure**	Mail.	
22218	Edward Solta & LAMP 1300 G		
	a. Blue Light: b. Red Light: c.	St. Dayling	that y


## Applicators and St

	and Shame
Catal	Specificaries Spare Parts
22002	SMALL ROUND OF MELS LENS APPLICATIONS LARGE SOFTARE QUARTE LENS APPLICATION MEDICAL ROUND QUARTE LESS APPLICATION
22003	
33,0414	Menten Rockly Order Than Applied the
22005	AFRICA ROUND OF ARTS LEAS APPLICATIONS  LARGE SOFTARE QUARTE LESS APPLICATION  MEDICAL ROUND QUARTE LESS APPLICATION  HEMORRHOID APPLICATION
22006	
22007	
22008	QUARTZ Ron, 63 " John Will Straight and " " "
22009	OUNCE Rob. 25 " long with straight end OUNCE Rob. 65 " long with straight end Brue "United Violet Glass" burnes, 2 3" [ ]
22010	MICA PROTECTING ACTIONS PRINTERS, 2, 3 July 1
22011	GUARTZ Ron, 63;" long with shaped and BEUE TURKA VIOLET GLASS" PHATERS, 2, 3, 4, 5 and 1992 WEAVER APPLICATOR RUBBER TURKS, Dec. Foot
22012	
22014	QUARTE LAMB WINDOW
22015	Of ARTZ LAMP WINDOW SHARDE LOCALIZER with 3 tubes SINUS APPLICATOR (McManus)
22016	SINUS APPLICATOR (Maximum and an annual an annual and an annual an ann
22017	SINUS APPLICATOR (McManus) PLASE PROCESSORS
22018	The Control of the Co
22019	BALDWIN LARYNGUSCOUP & Company of the Company of th
23024	Ballowin Laryncoscopy for Alpine Sun Lamp
22025	BURRONE & Proceedings of the Mannes of the Committee of t
22026	Del Billion   1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1 1
22027	MEHLER XXXXII XXIII III III III III III III I
22050	THE COURT OF THE C
23020	Plant the race of the control of the
53333	LANGUER QUARTE TRRUCKLINGS (Det page)
22120	LANSINGE THE STATE OF THE PARTY
2127	MAYER ALEXI APPER COMES, per set or con-
22128	WAGNER OF OTHER SPECIAL WARRENCE OF THE WAGNER OF THE SECOND OF THE SECO
12150	Which is Quarter Spiceria, per set of three
22152	McCaskiy's Phosiatio Arriver of three
1033	SAMPSON PARENTAL APPLICATIONS, Set of Star.
70.71	SAMPSON HAVE LAND APPENATORS, SELECTION SAMPSON LAND
7.51	Sampson Larrangement Applications Legendre Applications
2000	Territory Appear aring the Manager Property of the Control of the
3117	WALNUT PRIVATE OF REFERENCE OF THE
310	WAGNER PRISMANNE Report of the Control
	The former of the control of the first of the first of the control
	A STORY OF THE STO
	Special Montre President Vision Vision
	Diela Visa

175 00



An Ideal Equipment for the Busy Practitioner

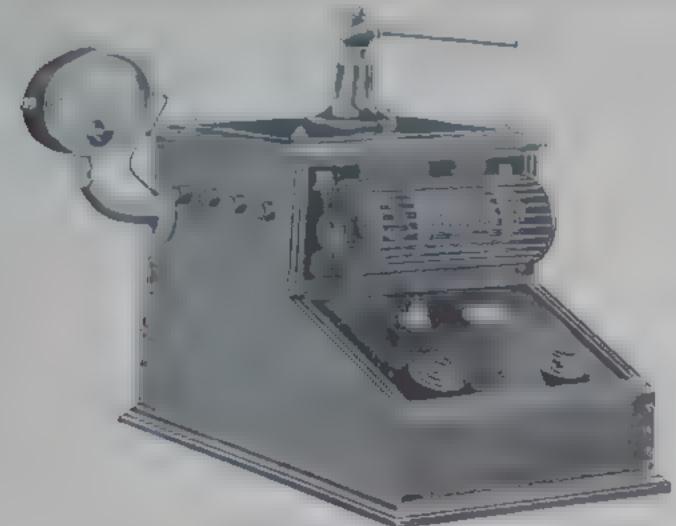

"CA" Diathermy


The requirements of Physical Therapy

are aptly met with an equipment including

Campbell Diathermy Generator

MODEL "CA" as illustrated above and

Morse Wave Generator

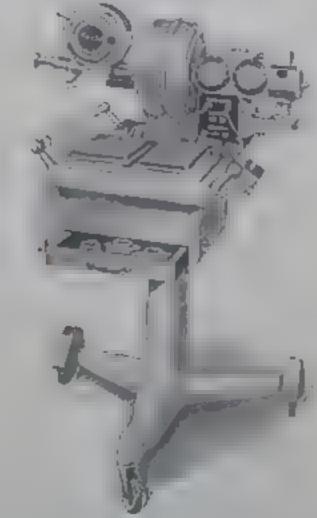

Morse Wave Generator





## Morse Wave Generator

Cutalog	sue SPECIFICATIONS	
Citizano	WALLESSE" WAVE OLD ERATOR, Technology of the con-	Price
21250	colt. 60 cycle current	
21351	Same at Cat. No. 21250 but for operation on 110 tota, D. C. Same as Cat. No. 21250 but for operation on 110	\$475 (ii)
31252	Same as Cat. No. 21250 but for operation on 110 colt, 50 cycle current	475:00
9253		475,00
21254	Same as Cat. No. 21250 but for operation on 110 volt, 25 cycle current	475 OF 475 OF
		77,5171
	Air and Vacuum Apparatus	
	Furnished in gray enamel finish as standard F. O. B. Cincinnati	
21150	Model, CS Ovirer, complete with suction and pressure models.	
21140	migral top, heater builds, one instrument tray, fiveg sprays one points	
	lizer, two powder blowers, and glass-stoppered medicine hopies (1)0-	
	V. 60 cycles 3. C	\$178.00
21151	Same as Cat. No. 21150 except for 220 V, 60 eyeles A, C.	180.00
21152	Same as Cat. No. 21150 except for 25, 30, 40 or 50 cycles it in car	185.00
51473	220 V. (specify cycles and voltage when ordering on this Cat. No.) Same as Cat. No. 21150 except for 110 V. D. C	178 00
21153	Same as Cat. No. 21150 except for 220 V. D. C	150 000
21154	Month, CG Outgir, including all the standard equipment of the Westel	
21160	CS, and in addition: Air Heater, large and small Surface, Rectal Dillo-	
	tor, Rectal Electrode, two Rubber Cups, Glass Breast Suction Cups and	P.S.LO
21161	Same as Cat. No. 21160, except for 220 V, 60 cycle- V Commun.	197.60
21162	20 April 19 April 20	
	Visit consider evelos and voltage when ordering on this U.H. No. 1	71.518
21163		
21164	Same as Cat. No. 21160 except for 220 V. D. C	
	Accessories for Above	
	enreirie ATIONS	Price
Catalo	ogue	
21170	Fitter VAPOR AND Section Octavit, consisting and a large sile order bottle with the necessary base and applicator, and a large sile order.	
	buttle will the necessary of a second buse and applicable.	3 11 3
	mounted on a heavy, non-tip metal base	
21171	mounted on a heavy, non-tip metal base  Sucrious Borrist, only, consisting of large size and applicator mounts on leavy	
21171		
	tip metal base	
21172		
	With mose prece directly connected and Sixus Charles and Constant Positive and Nagarity Sixus Charles and Constant Positive and Nagarity Sixus Charles and Constant Positive and Section Fortion for the Constant Positive Research and Constant Positive Research Resea	
21173	COMBINATION POSPINI ON ABBUTTON LORD TO STATE OF	
	trea halfies, one was a	-
	hottle and an arrangement of the Volts and Solar Volts and Sol	
18450	<ul> <li>Apr. Heaville with the Physics and April 10 Artists of the</li> </ul>	
18469	Powder Blower, and there Sterage Center	
	Powder Blower and Co.	

ements of

## Therapy


v met ent including

bell Generator

"CA"

d above

Generator

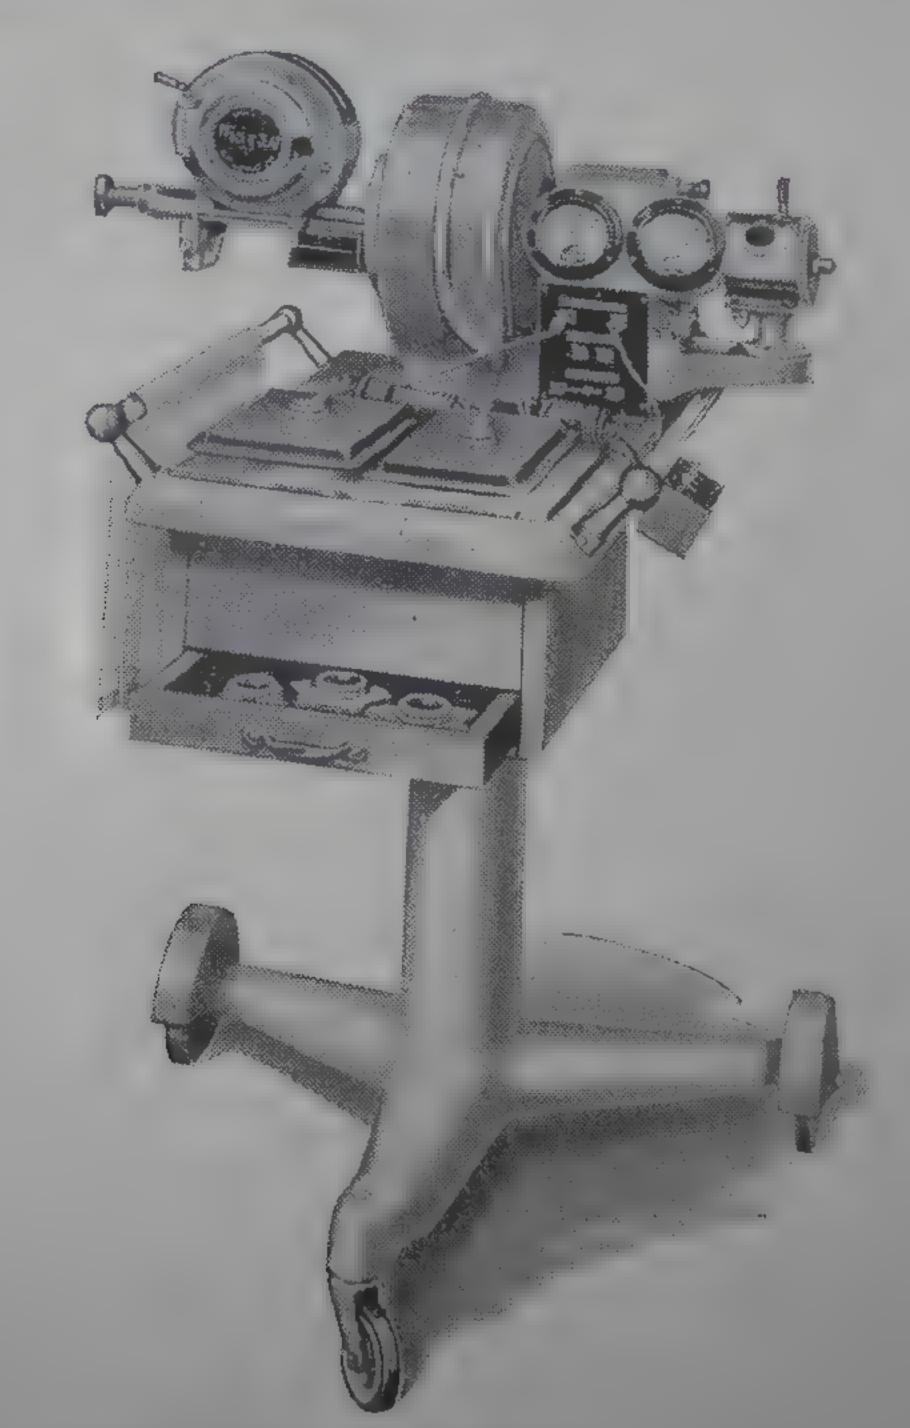

Morse Wave Generator

21 10 21 16

7

Cati


. . .

. . .

١.



# An Ideal Equipment for the Busy Practitioner

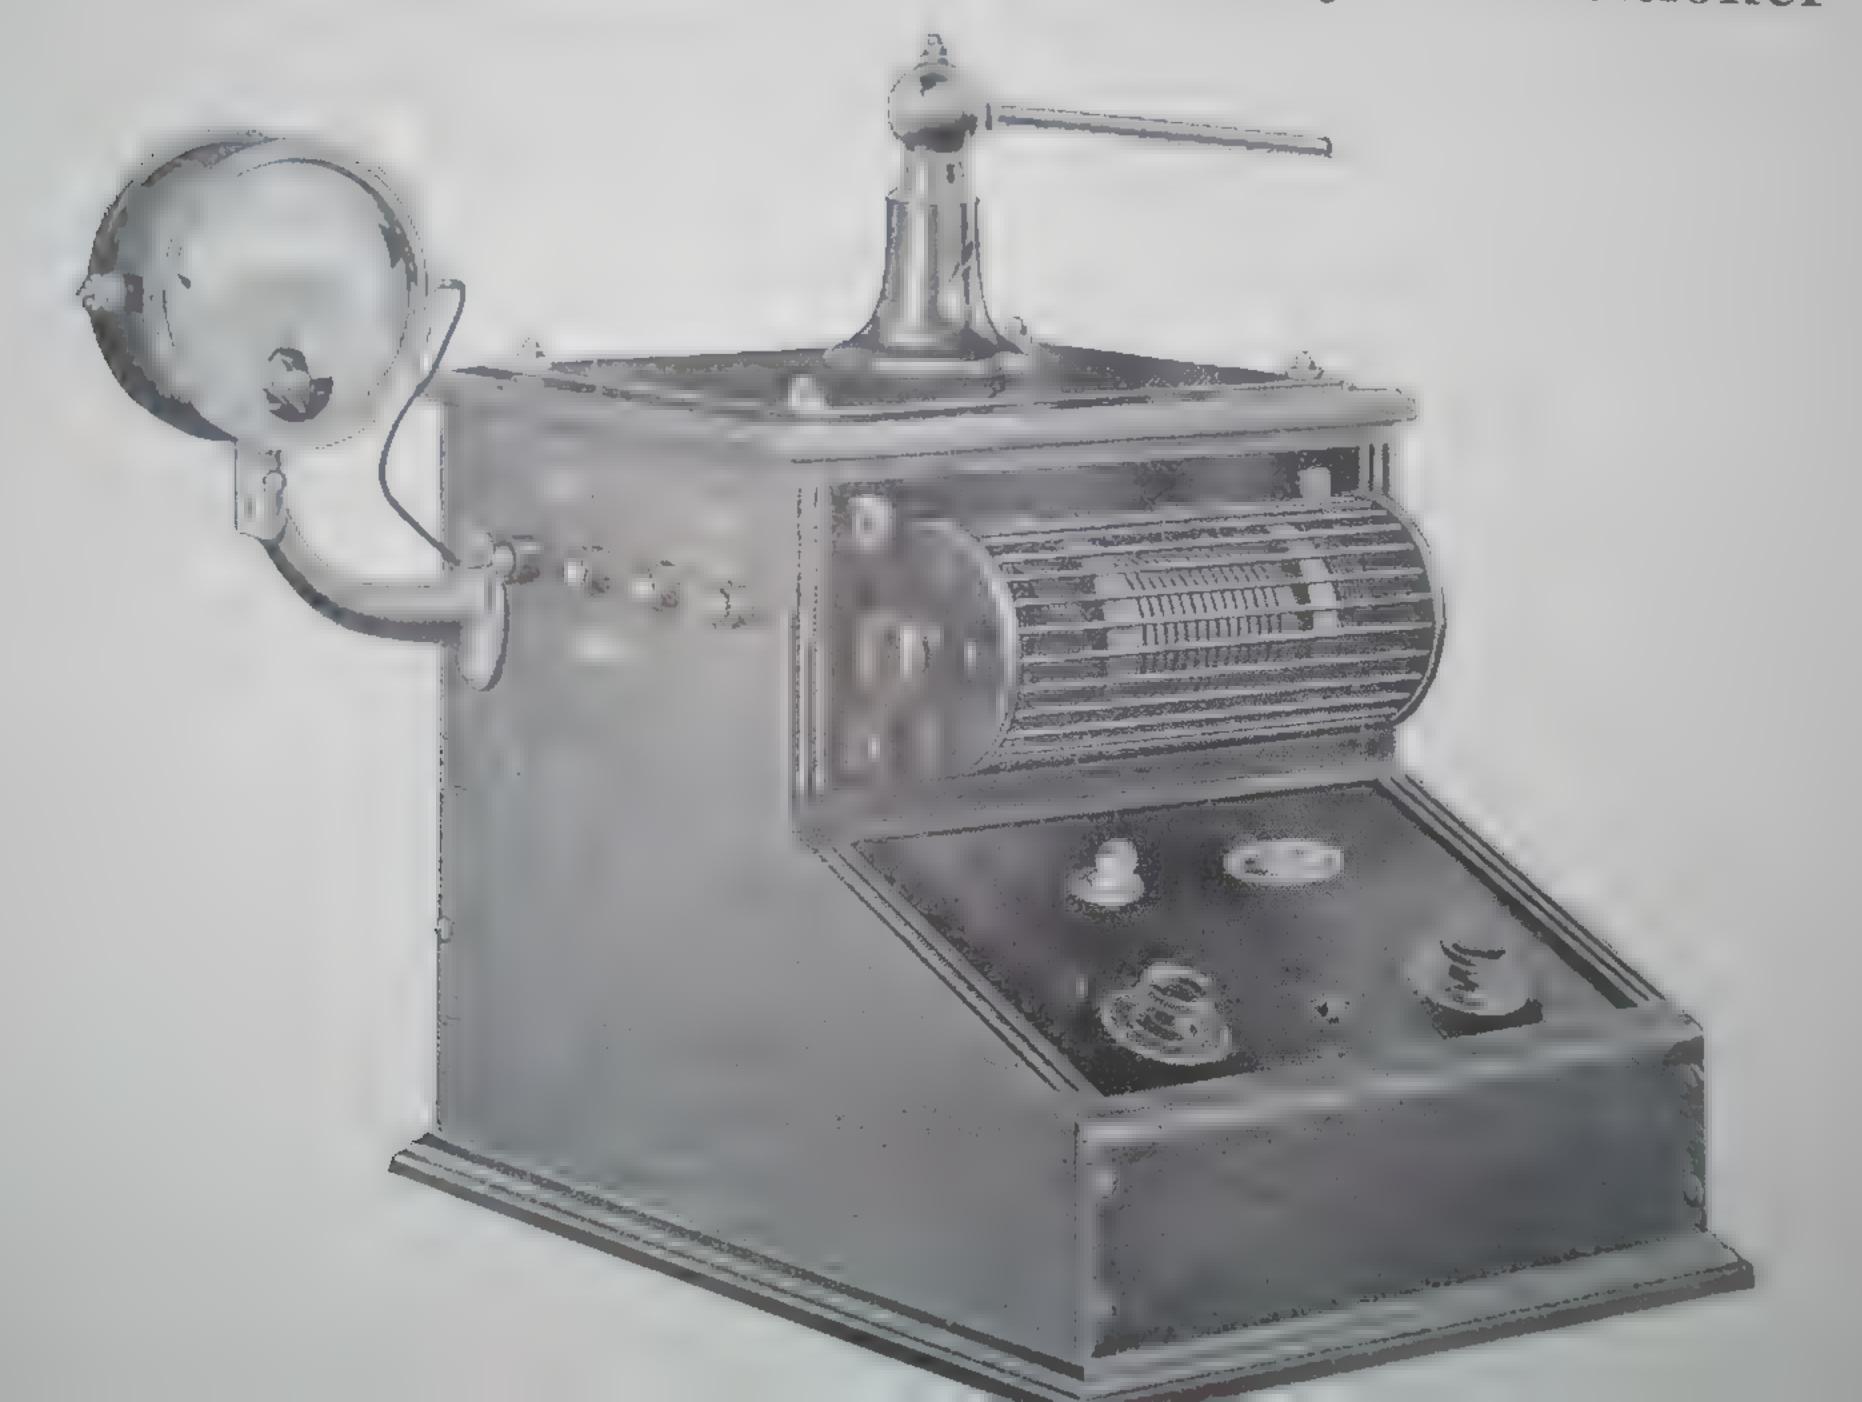



1898

1928

#### THIRTY YEARS OF PROGRESS WITH CAMPBELL



Model 1997

the aret increaseful N Roy and High Frequency Apparatus manufactured in the United States was built by CAMPRELL.

1898

Introduced to A. M. A. 1901.

ten ver states thousands of improved types were giving service to the medical profession.



Model "E"



Steady and constructive progress by Campbell engineers, produced the perfected combination X-Ray and Electro-Vedical equipment pictured to the left, many times copied but never equaled.

Modern on 10%, just there years since Compress, produced the first Diathermy the the first United States, there is an implied a complete line of efficient quality. It is common placed on pages 1 to 14 melusive of this booklet as well as four modern - 10, there is apparatus (pages 23 to 28 inclusive), producing every modern with hy to New Every of another of anything set offered. Send for catalogue.





## Two Views of the Factory that Serves You




Screw Machines

#### SIX-FLOOR MODERN CEMENT BUILDING



A Corner of Our Machine Shop

TRAINED OPERATIVES OF LONG EXPERIENCE




## Two views of the Factory that Serves You



Screw Machines

DOILDING

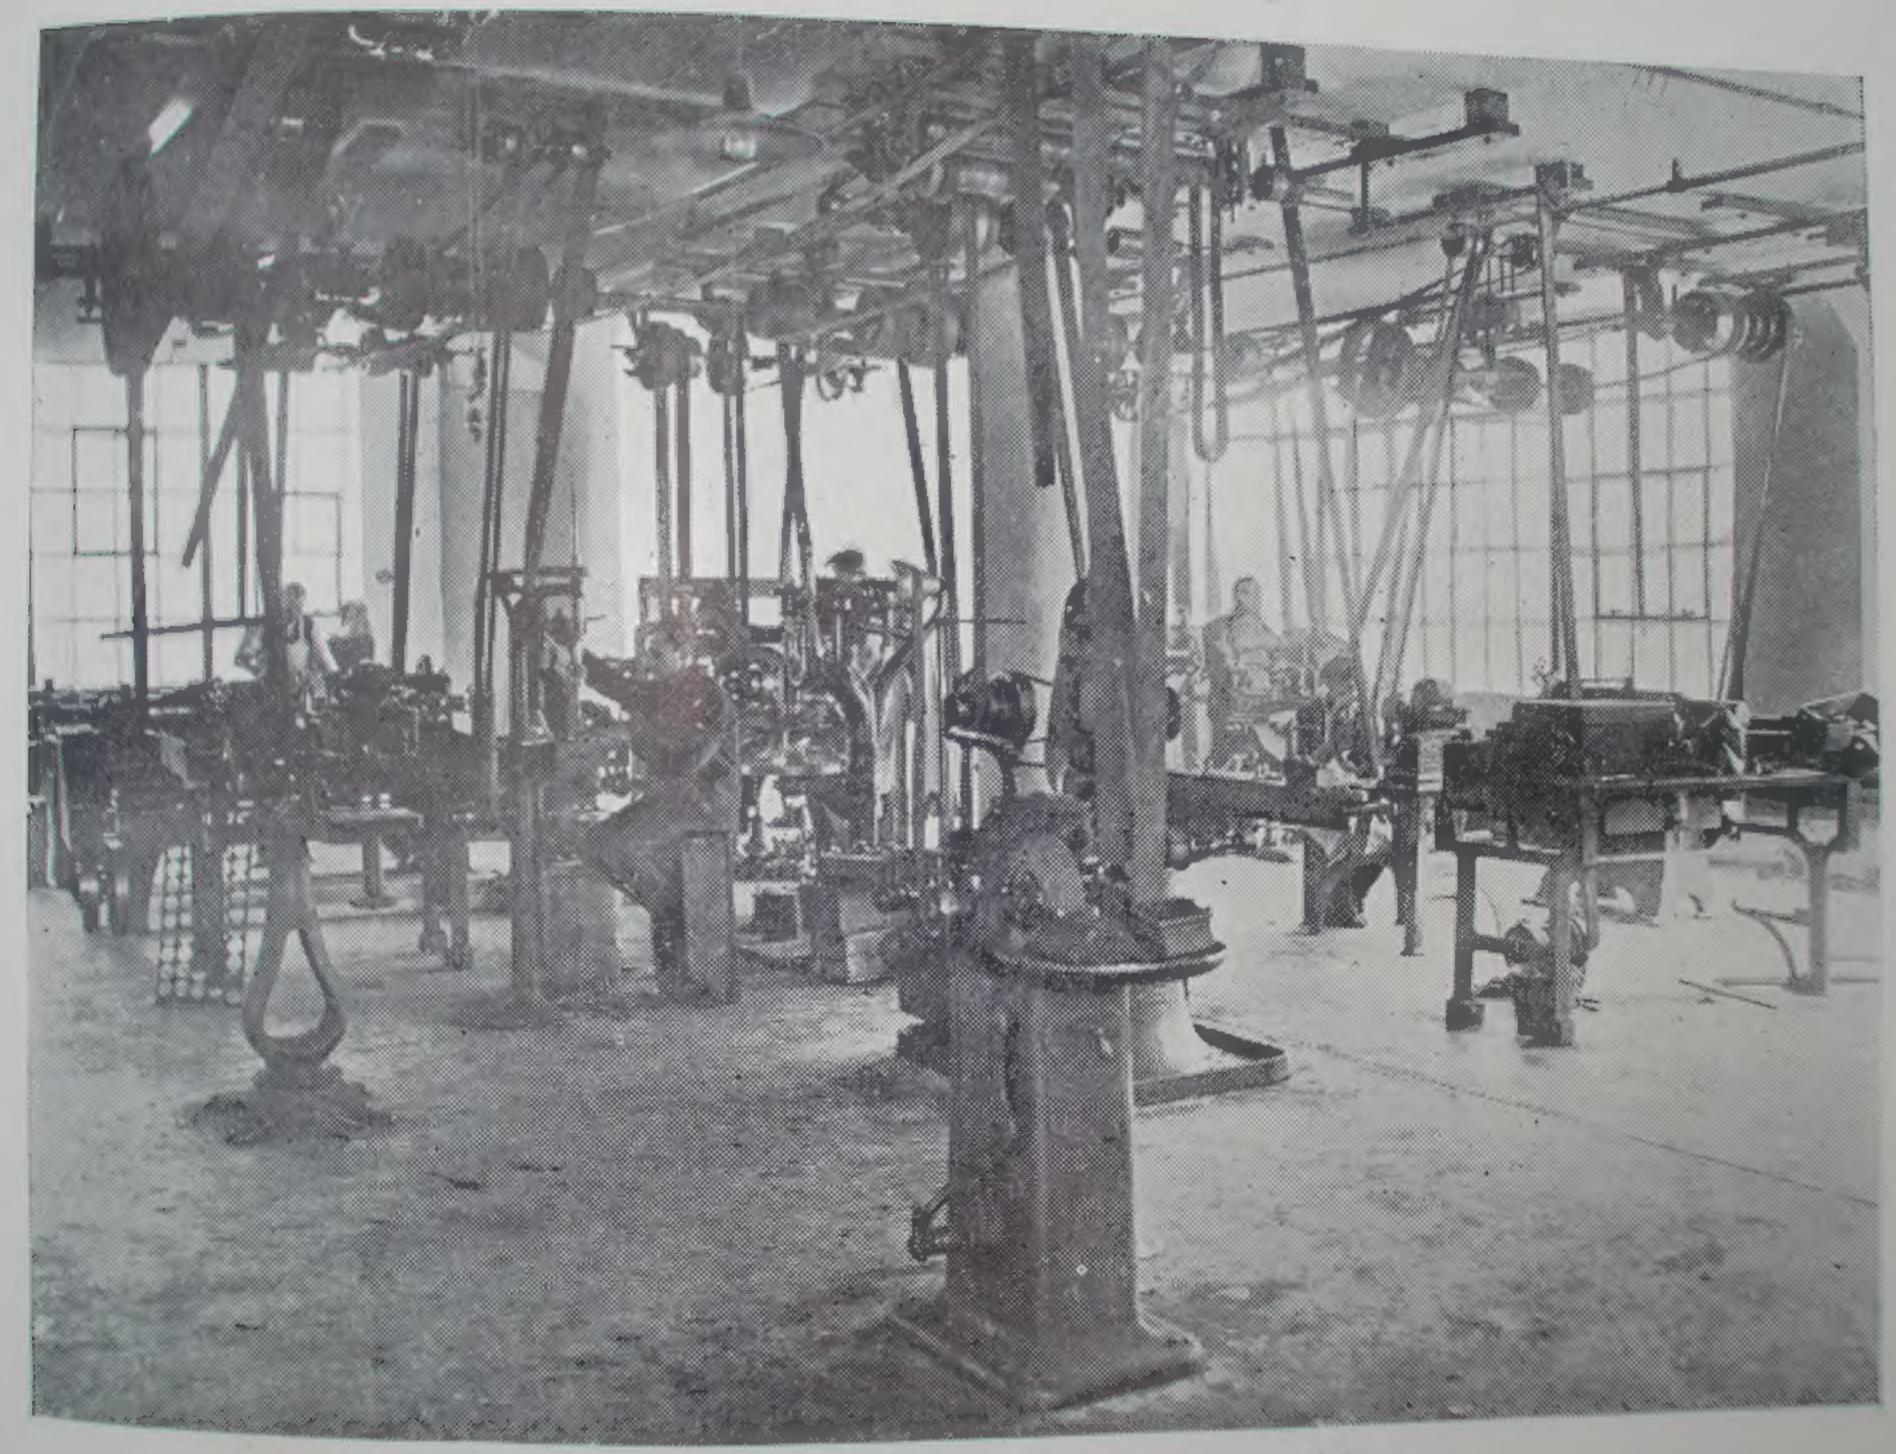

A Corner of Our Machine Shop





JULY 15, 1928

## PRICE LIST

# X-RAY AND PHYSICAL-THERAPY APPARATUS

ACCESSORIES AND SUPPLIES



All Prices Are F.O.B. Lynn, Mass. and subject to change without notice Always order by Catalogue number and give full description. Cash discount quoted on request

CAMPBELL ELECTRIC MFG. CO.

Campbell Building

15-19 Stewart Street

LYNN, MASSACHUSETTS